



**Customer:** Big Sky Scientific  
**Customer Sample ID:** Big Sky CBD Isolate  
**Laboratory Number:** 19H0215-01


## Cannabinoid Profile

**Extraction Technician:** RH  
**Analytical Chemist:** CB

Extraction Date(s)	Analysis Date(s)
8/20/2019	8/20/2019

Cannabinoids (HPLC)		Results	
	LOD (mg/g)	%	mg/g
Cannabidivarin (CBDV)	<1.90		
Cannabidiolic Acid (CBD-A)	<1.90		
Cannabigerolic Acid (CBG-A)	<1.90		
Cannabigerol (CBG)	<1.90		
Cannabidiol (CBD)		100.7	1010
Tetrahydrocannabivarin (THCV)	<1.90		
Cannabinol (CBN)	<1.90		
delta 9-Tetrahydrocannabinol (THC)	<1.90		
delta 8-Tetrahydrocannabidol	<1.90		
Cannabichromene (CBC)	<1.90		
delta-9-Tetrahydrocannabinolic Acid (THC-A)	<1.90		
Cannabinoids Total		%	mg/g
Max Active THC		0.00	0.00
Max Active CBD		101.00	1010.00
T.Active Cannabinoids		101	1010
Total Cannabinoids		101	1010
Ratios			
NA:1 CBD to THC		0.00:1 THC to CBD	

### Cannabinoid (mg/g)

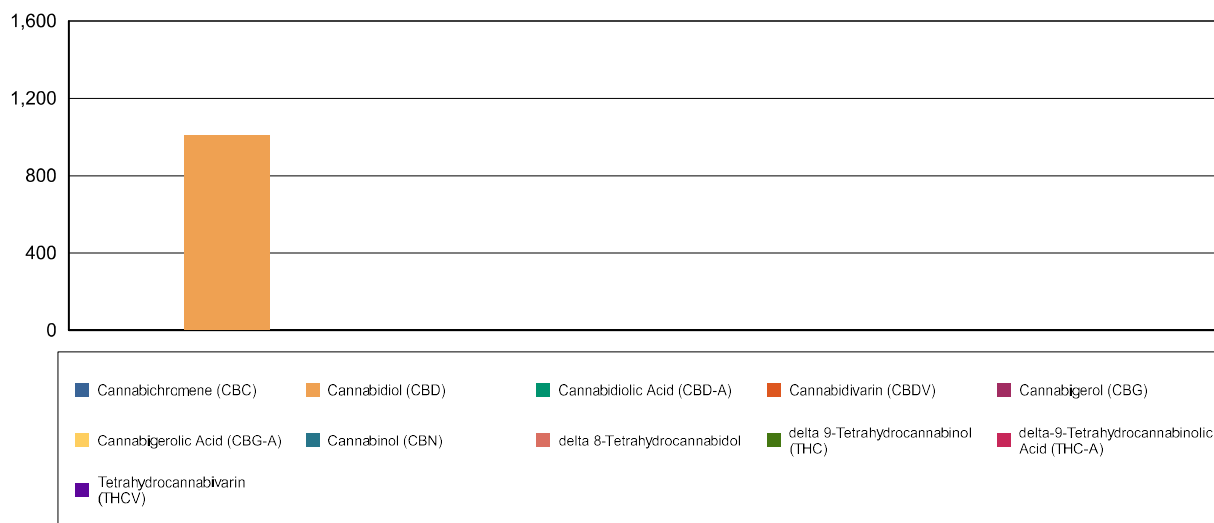

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods. The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.



**Customer:** Big Sky Scientific  
**Customer Sample ID:** Big Sky CBD Isolate  
**Laboratory Number:** 19H0215-01

## Residual Solvents Profile

**Extraction Technician:** RH  
**Analytical Chemist:** GB

Extraction Date(s)	Analysis Date(s)
8/20/2019	8/21/2019

Residual Solvents	Results	Calibration Range
	<b>ug/g</b>	
Propane	<96.3	100 - 2000
Isobutane	<96.3	100 - 2000
Methanol	<96.3	100 - 2000
Butane	<96.3	100 - 2000
Isopropanol	<96.3	100 - 2000
Ethanol	<96.3	100 - 2000
2-Methyl Butane	<96.3	100 - 2000
Acetonitrile	<96.3	100 - 2000
Acetone	<96.3	100 - 2000
n-Pentane	4920	100 - 2000
n-Hexane	<48.2	50 - 2000
Tetrahydrofuran	<96.3	100 - 2000
Benzene	<0.963	1.0 - 50
n-Heptane	<96.3	100 - 2000
Toluene	<96.3	100 - 2000
Ethylbenzene	<96.3	100 - 2000
m+p Xylene	<96.3	100 - 2000
o-Xylene	<96.3	100 - 2000
Total Xylenes	<96.3	100 - 2000
1,2,3-Trimethylbenzene	<96.3	100 - 2000

Altitude Consulting, LLC utilizes NIST traceable Reference Standards and Certified Reference Material to calibrate analytical instruments along with proven analytical methods .  
 The methods are applied in the most ethical manner following good laboratory practice guidelines. The results of this report are based solely on the sample submitted and cannot be reproduced.